


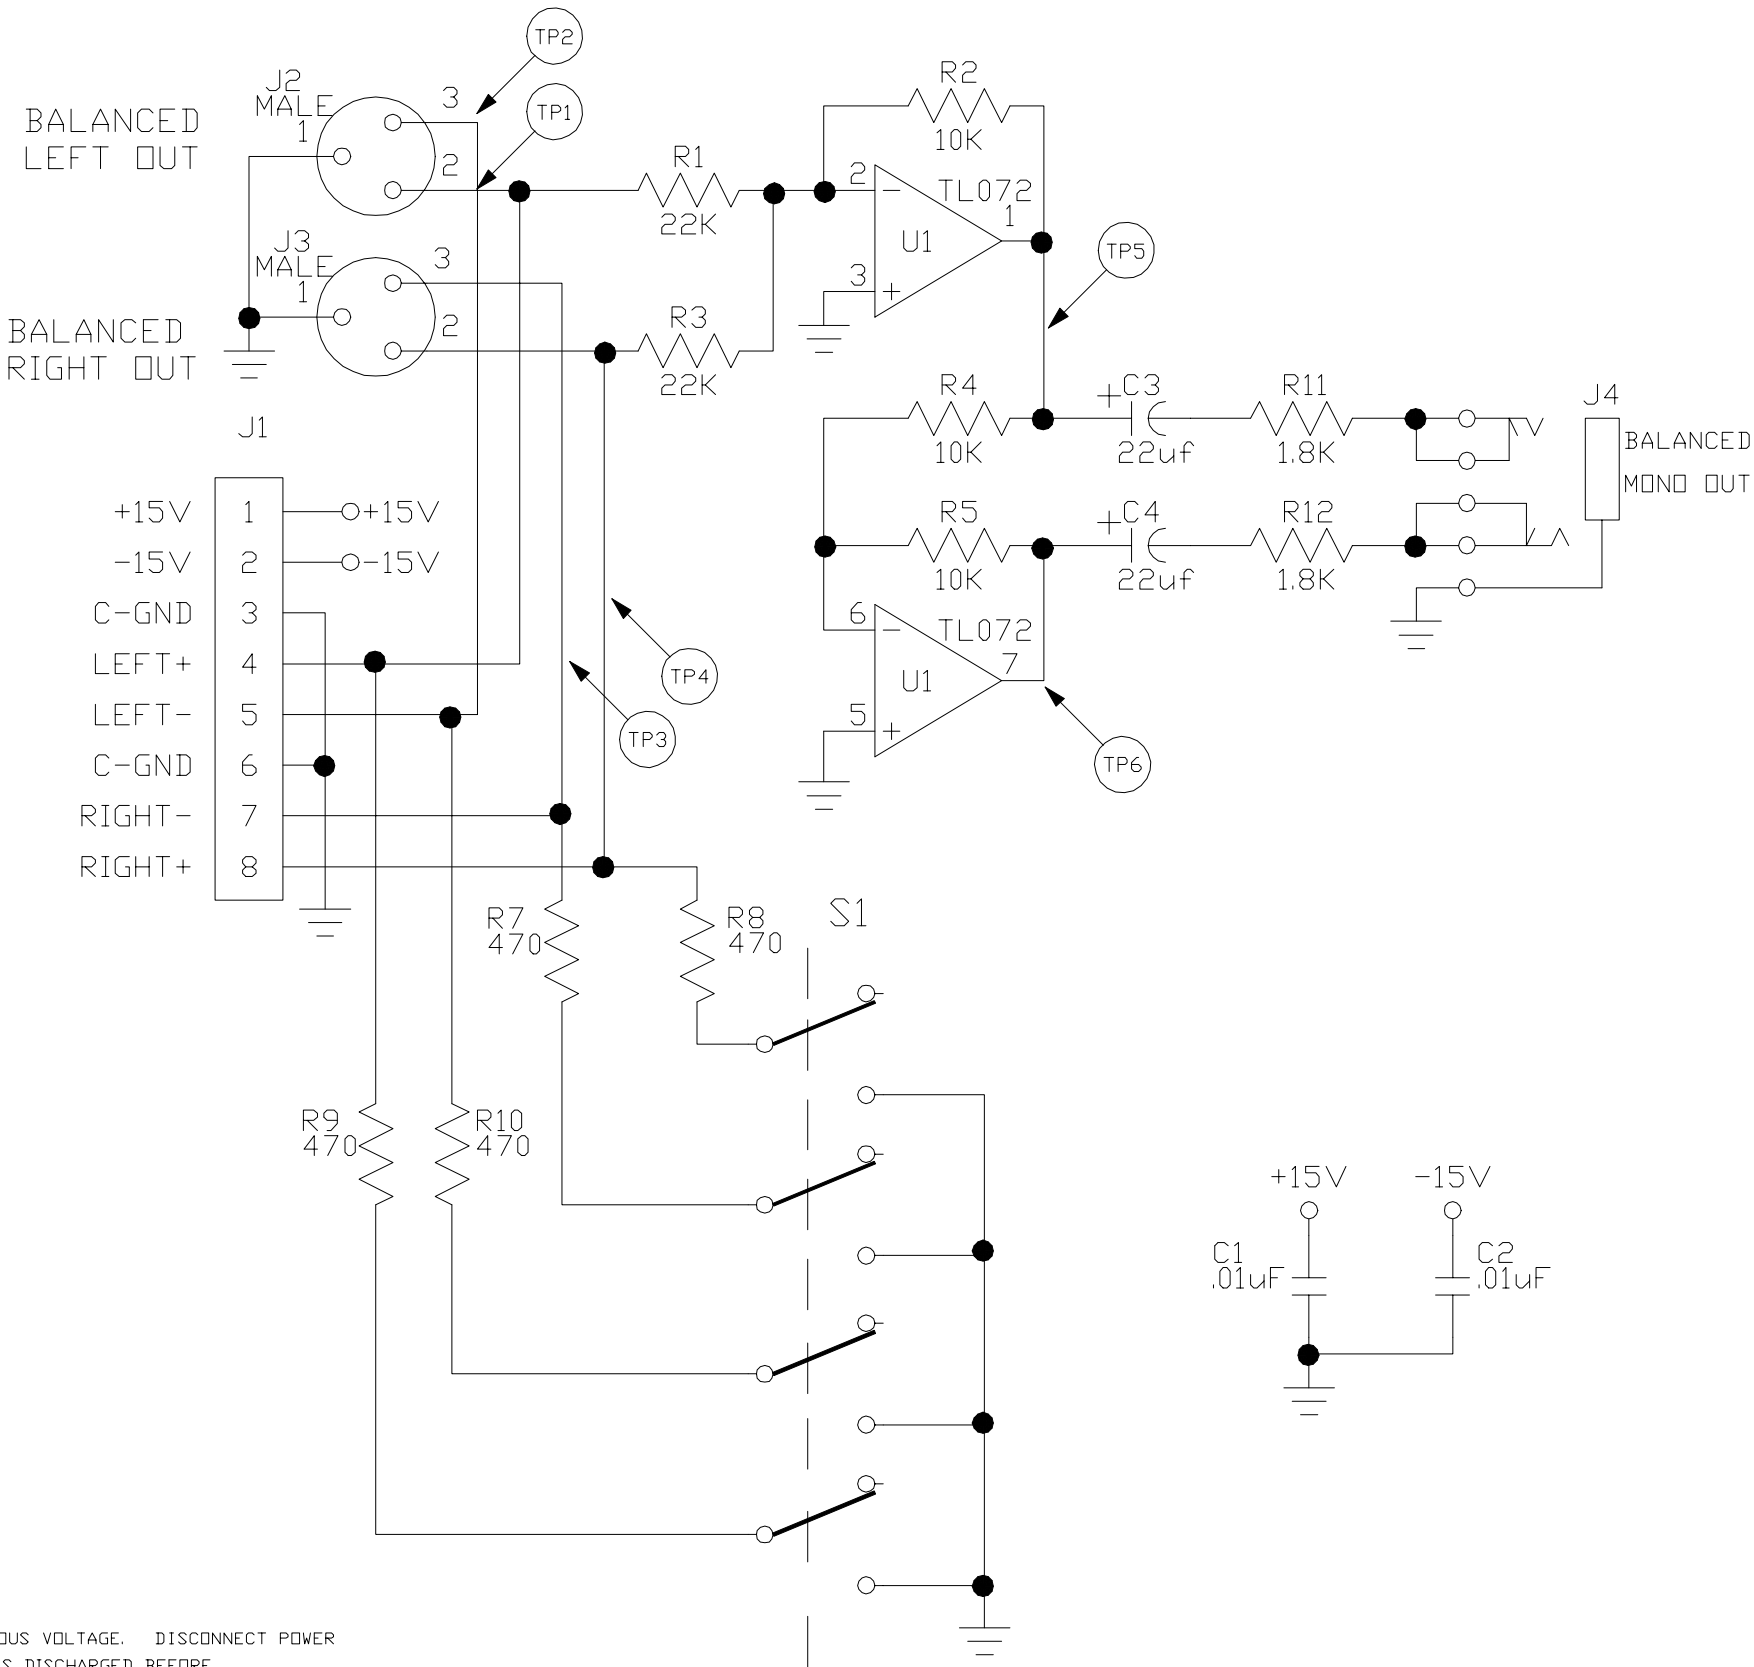

TEST POINTS	VOLTAGE
1	1 VAC
2	1 VAC
3	1 VAC
4	1 VAC
5	1 VAC
6	1 VAC
CONDITIONS SI IN OUT POSITION. IVAC APPLIED TO PINS 4, 5, 7, 8 OF J1	

TO RC1
OF 07-690-01

NOTES

- 1) CAUTION: SHOCK HAZARD!!
THIS UNIT CONTAINS HAZARDOUS VOLTAGE. DISCONNECT POWER AND BE SURE POWER SUPPLY IS DISCHARGED BEFORE TOUCHING INTERNAL PARTS.
- 2) UNLESS NOTED, RESISTOR VALUES IN OHMS, 1/4W-5% TOL. CAPACITOR VALUES IN MICROFARADS, 50V-10% TOL.
- 3) VOLTAGES ARE MEASURED WITH 1 MEGOHM OSCILLOSCOPE AND 10 MEGOHM DIGITAL VOLTMETER.
- 4) CHASSIS GROUND --- SIGNAL GROUND --- CIRCUIT GROUND ---

CAUTION:
THIS SCHEMATIC IS PROVIDED FOR USE BY QUALIFIED PERSONNEL. TO AVOID RISK OF ELECTRIC SHOCK, REFER SERVICING TO QUALIFIED SERVICE PERSONNEL. DO NOT PERFORM ANY SERVICING BEYOND THAT EXPLAINED IN THE OPERATING INSTRUCTIONS.

1				
2				
1	09/11/97	SWR		CHANGED P/N FOR S1 ON PICT., SCH. NOT AFFECTED. PER ECO #970500.
REV	DATE	BY	CHK'D	DESCRIPTION
SIGNATURES:			DATE:	 TERRY BORMAN DR. ST. LOUIS, MISSOURI 63146
DRAWN: MAG		05/13/97		
CHK'D: JJP		06/11/97		
APP'D: JJP		06/11/97		
ORIGINAL ISSUED:			06/11/97	
PLOT DATE:			09/11/97	
PLOT TIME:			08:41:42	
FILE NAME:			69101n1_	
PROJECT NAME:				ACM-1406
DRAWING NAME:				SCHEMATIC
DRAWING NO.				07H691-01
SCALE: 1:1				SHEET: 1 OF 1
				REV 1